



# Dovetail<sup>®</sup> HiChIP *MNase* Kit

## Mammalian Cells

### USER GUIDE

VERSION 2.0

CANTATA BIO, LLC.

100 ENTERPRISE WAY

SCOTTS VALLEY, CA 95066

(831) 233 - 3780

[SUPPORT@CANTATABIO.COM](mailto:SUPPORT@CANTATABIO.COM)

# Table of Contents

Copyright.....3

Dovetail® HiChIP *MNase* Kit Components and Storage.....4

Optional Add-on Modules: Components and Storage.....5

    Dovetail® Dual Index Primer Set #1 For Illumina.....5

    Dovetail® Library Module For Illumina.....5

User Supplied Reagents, Consumables and Equipment.....6

    Reagents.....6

    Consumables and Equipment.....6

Dovetail® HiChIP *MNase* Protocol Overview .....7

    Good Practices.....8

    Things to Consider Before You Start .....9

    Stage 1: Sample Preparation (Crosslinking, Digestion and Lysis) .....11

    Stage 2: Lysate QC.....16

    Stage 3: Chromatin Immunoprecipitation.....20

    Stage 4: Proximity Ligation .....23

    Stage 5: Library Preparation .....28

    Stage 6: Ligation Capture and Amplification.....32

    Sequencing & QC Analysis.....36

Appendix 1: Sample Preparation for 1 x 10<sup>6</sup> Cell Input .....37

Appendix 2: Dual Index Primers.....40

# Copyright

Use of this product is subject to compliance with applicable Cantata Bio, LLC terms and licensing requirements described at <https://dovetailgenomics.com/terms-and-conditions/>.

Dovetail®, Dovetail Genomics®, and HiRise® are trademarks of Dovetail Genomics, LLC, a wholly owned subsidiary of Cantata Bio, LLC, in the U.S. and/or other countries. Illumina®, HiSeq®, MiSeq®, MiniSeq®, iSeq®, NextSeq®, NovaSeq® are registered trademarks of Illumina, Inc. Beckman Coulter®, Agencourt® and SPRIselect® are trademarks or registered trademarks of Beckman Coulter, Inc. Qubit® are trademarks or registered trademarks of Thermo Fisher Scientific. TapeStation® and Bioanalyzer® Systems are registered trademarks of Agilent Technologies. Invitrogen® is a registered trademark of Thermo Fisher Scientific Inc.

This documentation shall be used only by Cantata Bio, LLC customers in connection with the use of the Dovetail® HiChIP MNase Kit, Dovetail® Library Module for Illumina, or Dovetail® Dual Index Primer Set #1 for Illumina® and shall not be used for any other purpose without the prior written consent of Cantata Bio, LLC.

This document, the associated kits and, their contents shall not be used, distributed or reproduced in whole or in part and/or otherwise communicated or disclosed without the prior written consent of Cantata Bio, LLC.

Prior to using Dovetail® HiChIP MNase Kit, these instructions must be read and understood by properly trained personnel. FAILURE TO FOLLOW THESE INSTRUCTIONS MAY RESULT IN FAILURE OF THE PRODUCT TO PERFORM AS EXPECTED, DAMAGE TO THE PRODUCT OR CUSTOMER SAMPLES, INJURY TO PERSONS, INCLUDING TO USERS OR OTHERS, AND DAMAGE TO OTHER PROPERTY. CANTATA BIO DOES NOT ASSUME ANY LIABILITY ARISING OUT OF THE IMPROPER USE OF THE DOVETAIL® HICHIP MNASE KIT. The contents of this product have been specifically designed to work together and are optimized for this protocol. Please do not make any substitutions.

The use of this product may require the buyer to obtain additional third-party intellectual property rights for certain applications. Safety Data Sheets are available at <https://dovetailgenomics.com/support/sds/>.

For Research Use Only. Not for use in diagnostics or diagnostic procedures.

© 2023 Cantata Bio, LLC. All rights reserved.

August 14, 2023

For technical customer support, please contact






[support@cantatabio.com](mailto:support@cantatabio.com)

+1 (831) 233-3780













## Dovetail® HiChIP *MNase* Kit Components and Storage

Each kit contains a sufficient supply of materials to perform 8 reactions. The Dovetail® HiChIP *MNase* Kit comes as two boxes. Store the boxes as listed below immediately upon receipt.

**Table 1. Dovetail® Chromatin Immunoprecipitation Core Box 1 (PN DG-CHIP-001)**

Components	Size	Cap Color	Label Color	Storage
10X Wash Buffer	30 mL Bottle			2°C to 8°C
NWB Solution	30 mL Bottle			
Protein A/G Beads	0.5 mL Tube			
Crosslink Reversal Buffer	2 mL Tube			
Streptavidin Beads	0.5 mL Tube			
10X RIPA	30 mL Bottle			
20% SDS	0.5 mL Tube			

**Table 2. Dovetail® Micro-C Module Box 2 (PN DG-NUC-001)**

Components	Tube/ Bottle Size	Cap Color	Label Color	Storage
MNase Enzyme Mix	0.5 mL Tube			-30°C to -10°C
10X Nuclease Digest Buffer	2 mL Tube			
100 mM MgCl <sub>2</sub>	0.5 mL Tube			
0.5 M EGTA	0.5 mL Tube			
End Polishing Enzyme Mix	0.5 mL Tube			
End Polishing Buffer	2 mL Tube			
5X Bridge Ligation Buffer	0.5 mL Tube			
Bridge Ligase	0.5 mL Tube			
Bridge	0.5 mL Tube			
Intra-Aggregate Ligation Enzyme Mix	0.5 mL Tube			
Intra-Aggregate Ligation Buffer	2 mL Tube			
Proteinase K	0.5 mL Tube			
250 mM DTT	0.5 mL Tube			
HotStart PCR Ready Mix	0.5 mL Tube			

\* If no color is specified for Label Color or Cap Color, a white or clear label/cap was used.

# Optional Add-on Modules: Components and Storage

## Dovetail® Dual Index Primer Set #1 For Illumina







Table 3. Dovetail® Dual Index PrimerSet #1 For Illumina® (PN DG-PRS-002)

Components	Size	Cap Color	Label Color	Storage
Unique Dual Index (UDI) Primer Pairs (x 8, different)	0.5 mL Tube			-30°C to -10°C

\* If no color is specified for Label Color or Cap Color, a white or clear label/cap was used.

## Dovetail® Library Module For Illumina

Table 4. Dovetail® Library Module For Illumina (PN DG-LIB-001)

Components	Size	Cap Color	Label Color	Storage
End Repair Enzyme Buffer	0.5 mL Tube			-30°C to -10°C
End Repair Enzyme Mix	0.5 mL Tube			
Ligation Enhancer	0.5 mL Tube			
Ligation Enzyme Mix	0.5 mL Tube			
Adaptor for Illumina	0.5 mL Tube			
USER Enzyme Mix	0.5 mL Tube			

\* If no color is specified for Label Color or Cap Color, a white or clear label/cap was used.

# User Supplied Reagents, Consumables and Equipment

## Reagents


Table 5. Reagents

Reagents	Supplier	Part Number
SPRIselect® Beads, 5 mL	Beckman Coulter	B23317
37% Formaldehyde Solution	Sigma-Aldrich	F8775
1X PBS, pH 7.4, 500 mL	Thermo Fisher Scientific	10010023
100% EtOH	Generic	N/A
UltraPure™ DNase / RNase-Free Distilled Water, 500 mL	Thermo Fisher Scientific	10977015
DSG (Disuccinimidyl Glutarate)	Thermo Fisher Scientific	A35392
DMSO (Dimethyl Sulfoxide, Anhydrous ≥ 99.99%)	Sigma-Aldrich	276855-100ML
cOmplete™ Protease Inhibitor Cocktail	Sigma-Aldrich	11697498001
TE pH 8.0	Thermo Fisher Scientific	AM9849

## Consumables and Equipment

Table 6. Consumables and Equipment

Consumables/Equipment	Supplier	Part Number
1.5 mL Low binding microcentrifuge tubes	Generic	
0.2 mL PCR tubes		
5.0 mL centrifuge tubes		
Pipets and pipet tips		
Magnetic separation rack for 0.2 mL and 1.5 mL tubes		
Agitating thermal mixer		
Thermal cycler		
Vortex mixer		
Centrifuge for 0.2 mL, 1.5 mL and 5 mL tubes		
Hemocytometer		
Qubit® Fluorometer	Thermo Fisher Scientific	Q33226
Qubit® dsDNA HS Assay Kit	Thermo Fisher Scientific	Q32854
Qubit® Assay Tubes	Thermo Fisher Scientific	Q32856
TapeStation System (Fragment Analyzer or Bioanalyzer)	Agilent	Various

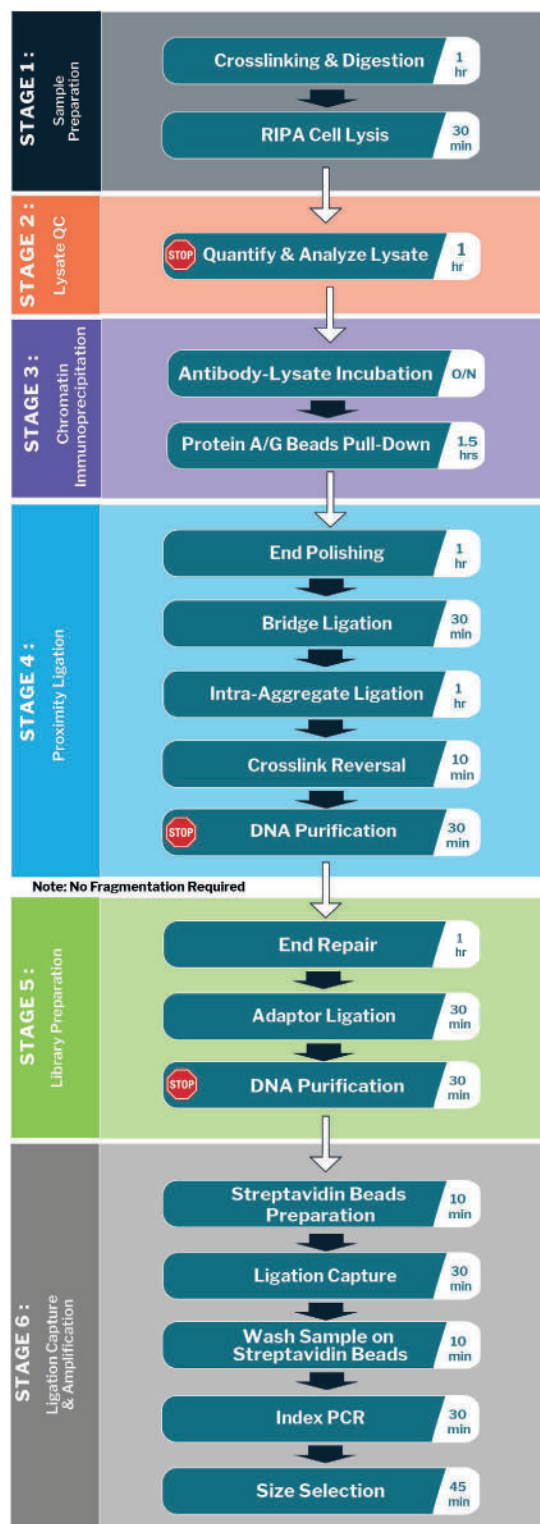Dovetail® HiChIP *MNase* Protocol Overview

## Good Practices

1. Read the entire guide before use, including Before You Begin and the Notes.
2. The cell input amount will influence the efficiency of the digestion reaction. To ensure an accurate cell count, use best practices such as low-speed spins ( $< 500 \times g$ ) using a swinging bucket rotor when harvesting the cells, and counting prior to freezing.
3. To ensure efficient crosslinking, a new or recently opened solution of formaldehyde should be used. Formaldehyde solution containing white precipitates should not be used.
4. Keep all enzymes and master mixes on ice during setup and use. Promptly move reagents back to the indicated storage.
5. Fully thaw buffers, place on ice and thoroughly mix before use.
6. When preparing master mixes, scale the volume of each reagent as appropriate, using 10% excess volume to compensate for pipetting loss.
7. Always add the reagents to the master mix in the specified order as listed throughout the protocol.
8. When working with beads, such as Protein A/G beads, SPRIselect and Streptavidin beads, you should:
  - a. Equilibrate the beads to room temperature before use.
  - b. Thoroughly vortex the beads immediately before use and ensure they are a homogeneous slurry.
  - c. When placing the tube in the magnetic rack, always wait until the solution looks clear to allow the beads to fully separate before removing the supernatant carefully and slowly. This helps minimize bead/sample loss throughout the protocol.
  - d. Do not let the beads dry out during washing steps. Keep the beads in buffer until ready to resuspend them for the next step.
  - e. After washing the SPRIselect beads with 80% ethanol during DNA purification, do not let the beads over-dry before proceeding with elution. Over-drying the beads may result in lower recovery of DNA.




## Things to Consider Before You Start

### How many cells should you start the assay with?

The number of cells to use for the HiChIP *MNase* assay can vary significantly depending on the cell type, the cell culture, and the abundance of the protein of interest. Please refer to the table below for the recommended starting cell number for your antibody of interest.

Antibody	Supplier	Part Number	Recommended amount (ng or $\mu$ L) of antibody	Recommended amount (ng) of chromatin	Recommended starting cell number
IgG	Cell Signaling	2729	Equivalent amount as the antibody of interest	Equivalent amount as the antibody of interest	Equivalent amount as antibody of interest
CTCF	Cell Signaling	3418	500 ng	1,000 - 1,500	$5 \times 10^6$
H3K4ac	Active Motif	39381	7.5 $\mu$ L	1,000 - 1,500	$5 \times 10^6$
H3K4me3	Cell Signaling	9751	1,250 ng	1,000 - 1,500	$5 \times 10^6$
H3K14ac	Cell Signaling	7627	4,000 ng	1,000 - 1,500	$5 \times 10^6$
H3K27ac	Cell Signaling	8173	300 ng	1,000 - 1,500	$5 \times 10^6$
H3K27ac	Millipore Sigma	MABE647	200 ng	1,000 - 1,500	$5 \times 10^6$
H3K27me3	Cell Signaling	9733	1,250 ng	1,000 - 1,500	$5 \times 10^6$
H3K36me3	Cell Signaling	4909	1,250 ng	1,000 - 1,500	$5 \times 10^6$
PollI	Abcam	ab26721	20,000 ng	1,000 - 1,500	$5 \times 10^6$
Klf4	Abcam	ab106629	20,000 ng	10,000	$10 \times 10^6$
Nanog	Abcam	ab21624	5,000 ng	10,000	$10 \times 10^6$
Oct4	Cell Signaling	2890	25 $\mu$ L	10,000	$10 \times 10^6$
Sox2	Cell Signaling	23064	500 ng	10,000	$10 \times 10^6$

 **NOTE** If you are using a non-Dovetail validated antibody, we recommend starting with  $10 \times 10^6$  cells.

**NOTES**

- » The first time you run the assay with a given cell type, we recommend to process a single cell aliquot through Stage 1 and Stage 2 to ensure the *MNase* digestion conditions are optimal for your cell type. Once the digestion conditions are optimized for your cell type, they are reproducible so you can set up multiple preparations in parallel.
- » If  $5 \times 10^6$  cells are not available, we recommend moving forward with the maximum number of cells obtainable and processing those in  $1 \times 10^6$  cell aliquots according to the  $1 \times 10^6$  cell sample preparation protocol. If you have fewer than  $1 \times 10^6$  cells, there is a high risk of not having sufficient yield to convert into a library or your library will have a high duplication rate and poor ChIP enrichment.

### Why is it important to achieve an optimal digestion?

Dovetail HiChIP *MNase* assay does not require sonication prior to library preparation. The fragmentation is solely based on enzymatic digestion with *MNase*. Achieving an optimal digestion profile which contains  $\geq 60\%$  mononucleosomes results in a high complexity library with enriched long-range interactions. When the chromatin is under-digested ( $< 60\%$  mononucleosomes), the library complexity is lower (i.e. higher duplication rate). In this case, you may need additional libraries to support the sequencing depth needed for your application.

### How much *MNase* enzyme should you use to achieve an optimal digestion?

The amount of *MNase* Enzyme Mix to use depends on the cell type and number. The appropriate *MNase* amount for your sample input and type may need to be optimized. The amounts provided in the User Guide are a general starting point.

Input	Enzyme Amount
$1 \times 10^6$ cells	0.5 $\mu$ L of <i>MNase</i> Enzyme Mix
$5 \times 10^6$ cells	2.5 $\mu$ L of <i>MNase</i> Enzyme Mix
$10 \times 10^6$ cells	5.0 $\mu$ L of <i>MNase</i> Enzyme Mix

### What is the sequencing depth and number of libraries needed?


The sequencing depth and number of libraries depend on your antibody/protein of interest and application. If your antibody of interest is CTCF, H3K27ac, or H3K4me3 and you are looking to call loops at 5 - 10 kb resolution, we recommend sequencing a pool of two libraries to a total of  $\sim 300$  M read pairs (2 x 150 bp). Please note that  $5 \times 10^6$  cells are typically sufficient for one HiChIP reaction and one library preparation.

## Stage 1: Sample Preparation (Crosslinking, Digestion and Lysis)

As you prepare for Stage 1, keep the following in mind:

- » Sample preparation takes ~ 1.5 hours.
- » Follow this sample preparation protocol if you are starting the assay with  $5 \times 10^6$  cells (Option A) or  $10 \times 10^6$  cells (Option B). If you are starting with  $1 \times 10^6$  cells, follow [Appendix 1: Sample Preparation for  \$1 \times 10^6\$  Cell Input](#), page 37.

Figure 1. Stage 1: Sample Preparation

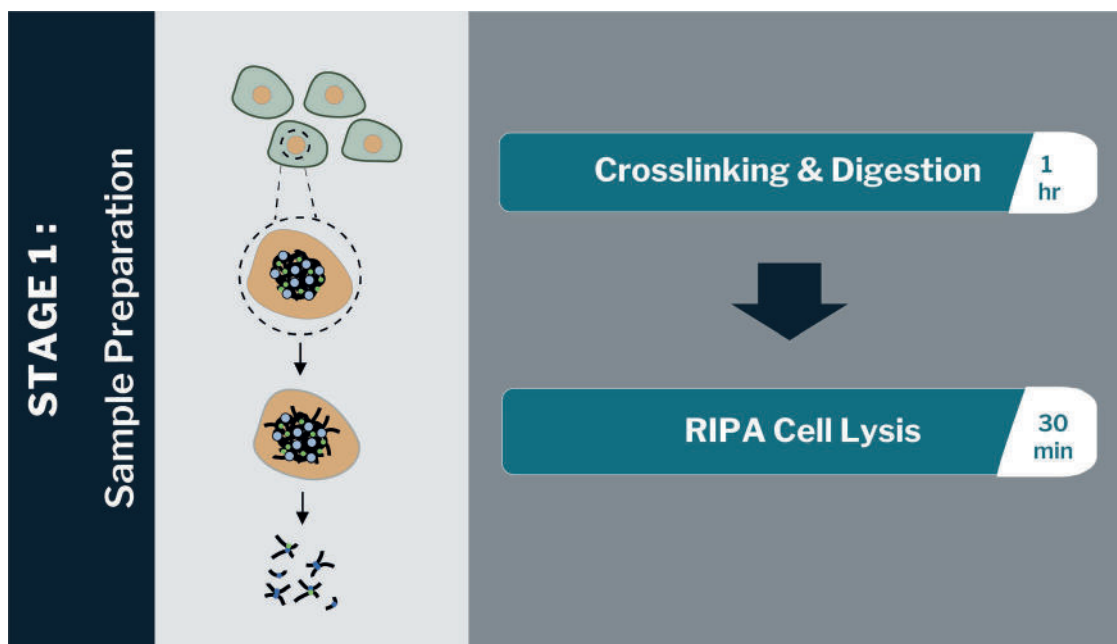

### Before You Begin

- » The 10X Wash Buffer and 20% SDS might have precipitated in storage. Incubate these solutions at 37°C for 15 minutes or until the precipitate is no longer visible. Vortex to mix prior to use.
- » Dilute 10X Wash Buffer to 1X with UltraPure™ Water. Store at room temperature. 1X Wash Buffer is stable at room temperature for 2 months. You need ~6 mL of 1X Wash Buffer per sample for the entire protocol.
- » Prepare 0.3 M DSG in DMSO (anhydrous) by dissolving 1 mg of DSG in 10.22  $\mu$ L DMSO. DSG is water-insoluble and moisture-sensitive. Prepare **immediately** before use. Do not store DSG in solution.
- » Prepare 25X Proteinase Inhibitors by dissolving 1 tablet of cOmplete™ Protease Inhibitor Cocktail in 2 mL of UltraPure™ Water and place on ice. The 25X Proteinase Inhibitors solution is stable at 4°C for 2 weeks.

- » Prepare fresh 1X Nuclease Digest Buffer and store at room temperature. 1X Nuclease Digest Buffer is stable for 1 day at room temperature. You need 100  $\mu$ L of 1X Nuclease Digest Buffer per sample. To prepare 1X Nuclease Digest Buffer (100  $\mu$ L), mix the following components:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	80 $\mu$ L	88 $\mu$ L	x	8	=	704 $\mu$ L
● 10X Nuclease Digest Buffer	10 $\mu$ L	11 $\mu$ L	x	8	=	88 $\mu$ L
● 100 mM MgCl <sub>2</sub>	10 $\mu$ L	11 $\mu$ L	x	8	=	88 $\mu$ L
<b>Total</b>	<b>100 <math>\mu</math>L</b>					

- » Set the thermal mixer at 22°C, shaking at 1,250 rpm.
- » Thaw ● 0.5 M EGTA at room temperature. Vortex to mix prior to use.

## Option A: If starting the assay with $5 \times 10^6$ cells

### 1.1 Crosslinking and Digestion

#### NOTES

- »  $5 \times 10^6$  cells are needed per HiChIP reaction.
- » Pre-freezing the cells is required to get an optimal digestion profile.
- » The cell pellet should be frozen at -80°C for at least 30 minutes (step 4). You can keep the cells frozen at -80°C for longer provided they are not subjected to freeze-thaw.
- » All crosslinking reactions (steps 5 – 12) should be carried out at room temperature.

#### Follow the steps below for Crosslinking and Digestion:

- Harvest the cells, wash with 1X PBS and count.
- Aliquot  $5 \times 10^6$  cells into a 1.5 mL tube.
- Spin the  $5 \times 10^6$  cell aliquot at 500 x g for 5 minutes in a swinging bucket rotor. Carefully remove and discard the supernatant.
- Freeze the cell pellet by placing it at -80°C for at least 30 minutes.
- Thaw your cell pellet quickly at room temperature then resuspend the pellet in 500  $\mu$ L of 1X PBS: first add 100  $\mu$ L of 1X PBS using a 100  $\mu$ L pipette. Pipet to break up clumps and then add the remaining 400  $\mu$ L. Pipet up and down to fully resuspend the pellet.
- Add 5  $\mu$ L of 0.3 M DSG. Pipet up and down to mix.
- Rotate the tube for 10 minutes at room temperature. Cells should not settle.
- Add 13.5  $\mu$ L of 37% formaldehyde.
- Rotate the tube for 10 minutes at room temperature. Cells should not settle.
- Spin the tube at 500 x g for 5 minutes in a swinging bucket rotor. Carefully remove and discard the supernatant. Use caution, the pellet might be loose.

## STAGE 1: SAMPLE PREPARATION (CROSSLINKING, DIGESTION AND LYSIS)

11. Wash the pellet with a total of 500  $\mu$ L 1X Wash Buffer: first add 100  $\mu$ L of 1X Wash Buffer using a 100  $\mu$ L pipette and pipet to break up clumps then add the remaining 400  $\mu$ L. Pipet up and down to fully resuspend the pellet.
12. Spin the tube at 500 x g for 5 minutes in a swinging bucket rotor. Carefully remove and discard the supernatant.
13. Repeat steps 11 and 12 once, for a total of 2 washes.
14. After removing the second wash, resuspend the cell pellet in 100  $\mu$ L 1X Nuclease Digest Buffer (freshly prepared, see Before You Begin, page 12).
15. Add 2.5  $\mu$ L of ● MNase Enzyme Mix. Pipet up and down to fully mix.
16. Incubate the tube at 22°C for exactly 15 minutes in an agitating thermal mixer set at 1,250 rpm. If you are working with a large number of samples, stagger the start of the digestion for each sample by 20 seconds then stop after corresponding 15 minutes.
17. Stop the reaction by adding 10  $\mu$ L of ● 0.5 M EGTA. Pipet up and down to fully mix.

## 1. 2 RIPA Cell Lysis

Follow the steps below for RIPA Cell Lysis:

1. Add to the sample tube 87.5  $\mu$ L of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	58.5 $\mu$ L	64.35 $\mu$ L	x	8	=	514.8 $\mu$ L
● 10X RIPA	20 $\mu$ L	22 $\mu$ L	x	8	=	176 $\mu$ L
25X Protease Inhibitors	8 $\mu$ L	8.8 $\mu$ L	x	8	=	70.4 $\mu$ L
● 20% SDS	1 $\mu$ L	1.1 $\mu$ L	x	8	=	8.8 $\mu$ L
<b>Total</b>	87.5 $\mu$ L					

2. Vortex the tube to mix three times for 5 seconds each.
3. Rotate the tube at room temperature for 15 minutes.
4. Spin the tube at 16,000 x g for 2 minutes.
5. Transfer the **SUPERNATANT (clarified lysate)** to a new 1.5 mL tube. This lysate contains the digested chromatin.
6. Continue to [Stage 2: Lysate QC, page 16](#).

## Option B: If starting the assay with $10 \times 10^6$ cells

### 1.1 Crosslinking and Digestion

#### NOTES

- »  $10 \times 10^6$  cells are needed per HiChIP reaction.
- » Pre-freezing the cells is required to get an optimal digestion profile.
- » The cell pellet should be frozen at  $-80^\circ\text{C}$  for at least 30 minutes (step 4). You can keep the cells frozen at  $-80^\circ\text{C}$  for longer provided they are not subjected to freeze-thaw.
- » All crosslinking reactions (steps 5 – 12) should be carried out at room temperature.

#### Follow the steps below for Crosslinking and Digestion:

1. Harvest the cells, wash with 1X PBS and count.
2. Aliquot  $10 \times 10^6$  cells into a 1.5 mL tube.
3. Spin the  $10 \times 10^6$  cell aliquot at 500 x g for 5 minutes in a swinging bucket rotor. Carefully discard the supernatant.
4. Freeze the cell pellet by placing it at  $-80^\circ\text{C}$  for at least 30 minutes.
5. Thaw your cell pellet quickly at room temperature then resuspend the pellet in 1 mL of 1X PBS: first add 200  $\mu\text{L}$  of 1X PBS using a 200  $\mu\text{L}$  pipette and pipet to break up clumps then add the remaining 800  $\mu\text{L}$ . Pipet up and down to fully resuspend the pellet.
6. Add 10  $\mu\text{L}$  of 0.3 M DSG. Pipet up and down to mix.
7. Rotate the tube for 10 minutes at room temperature. Cells should not settle.
8. Add 27  $\mu\text{L}$  of 37% formaldehyde.
9. Rotate the tube for 10 minutes at room temperature. Cells should not settle.
10. Spin the tube at 500 x g for 5 minutes in a swinging bucket rotor. Carefully discard the supernatant. Use caution, the pellet might be loose.
11. Wash the pellet with a total of 1 mL 1X Wash Buffer: first add 200  $\mu\text{L}$  of 1X Wash Buffer using a 200  $\mu\text{L}$  pipette and pipet to break up clumps, then add the remaining 800  $\mu\text{L}$ . Pipet up and down to fully resuspend the pellet.
12. Spin the tube at 500 x g for 5 minutes in a swinging bucket rotor. Carefully discard the supernatant.
13. Repeat steps 11 and 12 once, for a total of 2 washes.
14. After removing the second wash, resuspend the cell pellet in 100  $\mu\text{L}$  1X Nuclease Digest Buffer (freshly prepared, see Before You Begin, page 12).
15. Add 5  $\mu\text{L}$  of ● MNase Enzyme Mix. Pipet up and down to fully mix.
16. Incubate the tube at  $22^\circ\text{C}$  for exactly 15 minutes in an agitating thermal mixer set at 1,250 rpm. If you are working with a large number of samples, stagger the start of the digestion for each sample by 20 seconds then stop after corresponding 15 minutes.
17. Stop the reaction by adding 10  $\mu\text{L}$  of ● 0.5 M EGTA. Pipet up and down to fully mix.

## 1.2 RIPA Cell Lysis

Follow the steps below for RIPA Cell Lysis:

1. Add to the sample tube 85  $\mu$ L of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	56 $\mu$ L	61.6 $\mu$ L	x	8	=	492.8 $\mu$ L
● 10X RIPA	20 $\mu$ L	22 $\mu$ L	x	8	=	176 $\mu$ L
25X Protease Inhibitors	8 $\mu$ L	8.8 $\mu$ L	x	8	=	70.4 $\mu$ L
● 20% SDS	1 $\mu$ L	1.1 $\mu$ L	x	8	=	8.8 $\mu$ L
<b>Total</b>	<b>85 <math>\mu</math>L</b>					

2. Vortex the tube to mix three times for 5 seconds each.
3. Rotate the tube at room temperature for 15 minutes.
4. Spin the tube at 16,000 x g for 2 minutes.
5. Transfer the **SUPERNATANT (clarified lysate)** to a new 1.5 mL tube. This lysate contains the digested chromatin.
6. Continue to [Stage 2: Lysate QC, page 16](#).


## Stage 2: Lysate QC

As you prepare for Stage 1, keep the following in mind:

- » The Lysate QC stage takes ~ 1 hour.
- » This stage has 2 objectives:
  - » Quantify the clarified lysate.
  - » Confirm that the chromatin was properly digested.
- » The protocol below is written for the TapeStation; however, it is also compatible with the Bioanalyzer System and Fragment Analyzer. Please refer to the table below for the recommended kits for each system.

System	Recommended Kits
TapeStation	HS D5000
Bioanalyzer System	HS DNA
Fragment Analyzer	DNF-488 HS Genomic DNA

Figure 2. Stage 2: Lysate QC

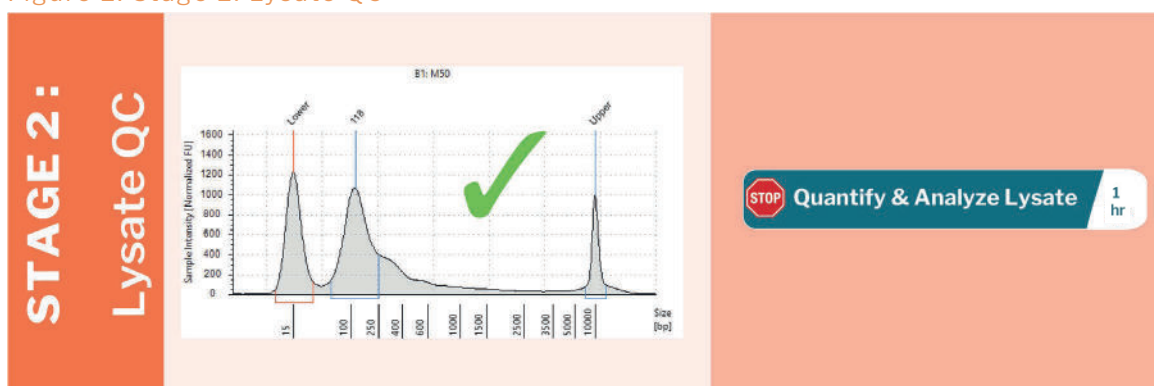

### Before You Begin

- » Prepare fresh 80% ethanol for DNA purification with SPRIselect beads for optimal results. Fresh preparations of 80% ethanol will also be used in the remaining stages, 5 and 6. You need a minimum of 1.5 mL for all these stages.
- » Program the thermal mixer as follows:

Temperature	Time
78°C	10 minutes
25°C	Hold



- » The ● Crosslink Reversal Buffer might have precipitated in storage. Incubate at 37°C for 15 minutes or until the precipitate is no longer visible. Vortex to mix prior to use.

### Follow the steps below for Lysate QC:

1. Transfer X  $\mu\text{L}$  of the clarified lysate (see table below) to a new 1.5 mL tube labeled QC.

Cell Input Amount	Clarified Lysate Volume (X) To Use For QC
$1 \times 10^6$ cells	10 $\mu\text{L}$
$5 \times 10^6$ cells	2.5 $\mu\text{L}$
$10 \times 10^6$ cells	2.5 $\mu\text{L}$

**NOTE** Store the remainder of the lysate on ice. This is the lysate you will be using in Stage 3. If you are not going to proceed with Stage 3 on the same day, store the remainder of the lysate at -80°C.

2. Add to the QC tube 51.5  $\mu\text{L}$  of a master mix containing the following reagents **in the order listed**:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
● Crosslink Reversal Buffer	50 $\mu\text{L}$	55 $\mu\text{L}$	x	8	=	440 $\mu\text{L}$
● Proteinase K	1.5 $\mu\text{L}$	1.7 $\mu\text{L}$	x	8	=	13.6 $\mu\text{L}$
<b>Total</b>	<b>51.5 <math>\mu\text{L}</math></b>					

3. Pipet up and down to fully mix. Incubate the QC tube in an agitating thermal mixer set at 1,250 rpm as follows:

Temperature	Time
78°C	10 minutes
25°C	Hold

4. Vortex the SPRIselect beads thoroughly (>30 seconds) to resuspend. Add 90  $\mu\text{L}$  of resuspended SPRIselect beads to the 1.5 mL tube containing your sample.
5. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
6. Incubate the tube at room temperature, off the magnetic rack, for 10 minutes.
7. Quick spin the tube and place it in the magnetic rack for 5 minutes. Discard the supernatant.
8. Leave the tube in the magnetic rack and wash the beads twice with 200  $\mu\text{L}$  fresh 80% ethanol. Do not resuspend the beads for these washes. Add the ethanol, wait for 1 minute then discard the ethanol supernatant.
9. After the last wash, quick spin the tube and place it in the magnetic rack for 1 minute. Use a 10  $\mu\text{L}$  pipet tip to remove traces of ethanol.
10. Air dry the beads in the magnetic rack for 5 minutes until no residual ethanol remains. Do not over dry the beads.
11. Off the magnetic rack, resuspend the beads in 10  $\mu\text{L}$  TE Buffer pH 8.0.

12. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
13. Incubate at room temperature, off the magnetic rack, for 5 minutes.
14. Quick spin the tube and place it in the magnetic rack for 1 minute (or until the solution looks clear).
15. Transfer 8  $\mu\text{L}$  of the SUPERNATANT (purified DNA) to a new tube. This new tube contains your purified QC DNA. Discard the beads.
16. Quantify 5  $\mu\text{L}$  of your purified QC DNA with a Qubit® Fluorometer and Qubit® dsDNA HS Kit. As a reference, we typically recover approximately 250 ng, 1,500 ng, and 3,000 ng from  $1 \times 10^6$ ,  $5 \times 10^6$ , and  $10 \times 10^6$  GM12878 cells, respectively.

» Based on the Qubit concentration, your total clarified lysate amount (ng) can be calculated as follows:

**If starting with  $1 \times 10^6$  cell input:**

» Total Clarified Lysate (ng) = Qubit reading ng/ $\mu\text{L}$  x 10  $\mu\text{L}$  (elution volume) x 20 (dilution factor)

**If starting with  $5 \times 10^6$  or  $10 \times 10^6$  cell input:**

» Total Clarified Lysate (ng) = Qubit reading ng/ $\mu\text{L}$  x 10  $\mu\text{L}$  (elution volume) x 80 (dilution factor)

**NOTE** If the clarified lysate yield is less than the recommended input for HiChIP with your antibody of interest (see [Things to Consider Before You Start, page 9](#)), there are 2 options for how to proceed:

**Option 1:** After completing Stage 2 and confirming that the chromatin is optimally digested, freeze the lysate at  $-80^\circ\text{C}$ . To reach the recommended clarified lysate amount, prepare additional lysate (run Stage 1 with a new cell aliquot), assess the digestion profile (Stage 2), and combine the lysates that are optimally digested before incubating with the antibody (Stage 3).


**Option 2:** If you still wish to proceed with less than the recommended lysate amount, please note that the library complexity will be reduced (i.e. the library will have a high duplication rate) and you may get poor ChIP enrichment

17. Check the fragment size distribution of your purified QC sample on a TapeStation HS D5000 ScreenTape. **Make sure your sample is diluted to 1 ng/ $\mu\text{L}$  to avoid overloading the tape which results in a misrepresentation of the fragment size distribution.**

- » The digestion profile should contain  $\geq 60\%$  mononucleosomes: the first DNA peak, typically in the size range of 50 - 250 bp for the TapeStation, should account for  $\geq 60\%$  of total DNA (Figure 3). The size range of the first peak may vary for other analytical instruments such as Bioanalyzer and Fragment Analyzer. If the digestion profile contains  $\geq 60\%$  mononucleosomes, proceed to [Stage 3: Chromatin Immunoprecipitation, page 20](#).
- » If the digestion profile contains  $< 60\%$  mononucleosomes, the chromatin is under-digested (Figure 3). When the chromatin is under-digested, the library complexity is lower (i.e. higher duplication rate). If you wish to proceed with the under-digested lysate, you may need additional libraries to support the sequencing depth needed for your application.

Alternatively, you can prepare a new lysate by re-running Stage 1 with a new cell aliquot, and increasing the MNase volume to achieve a profile with  $\geq 60\%$  mononucleosomes. If you need help with digestion optimization, please contact [support@cantatabio.com](mailto:support@cantatabio.com).

Figure 3. Different MNase digestion profiles, as analyzed on HS D5000 ScreenTape

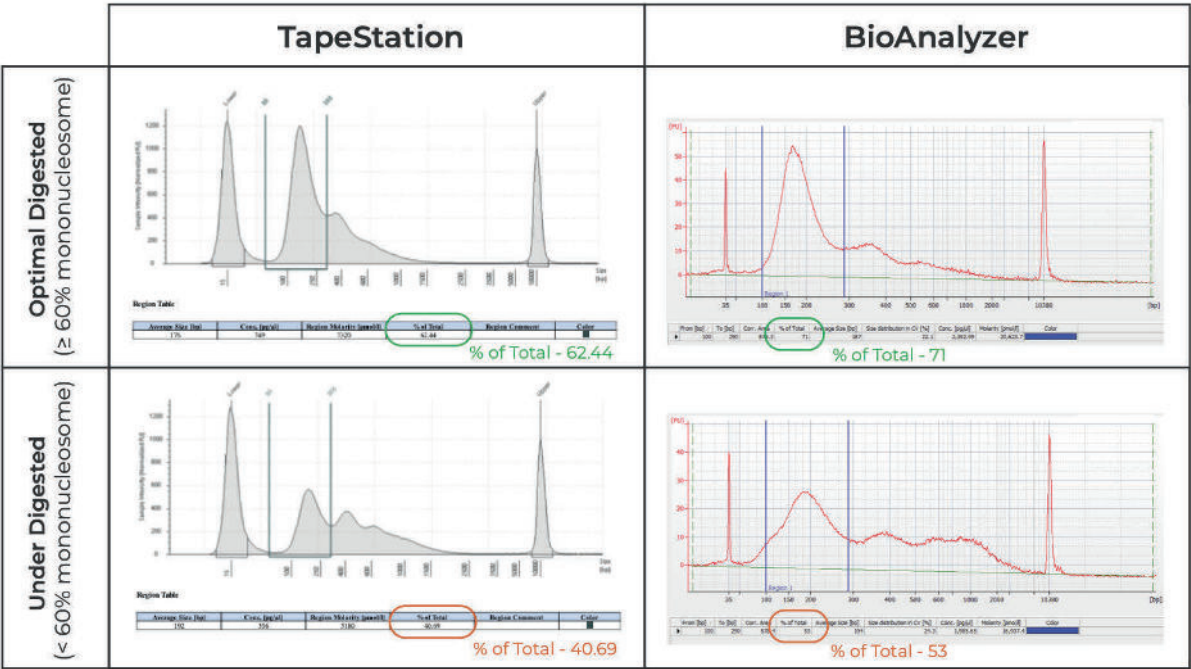


## Stage 3: Chromatin Immunoprecipitation

As you prepare for Stage 3, keep the following in mind:

- » Follow best practices when working with beads (see [Good Practices, page 8](#)).
- » The amount of antibody to add to the lysate is dependent on the antibody of interest.

Figure 4. Stage 3: Chromatin Immunoprecipitation

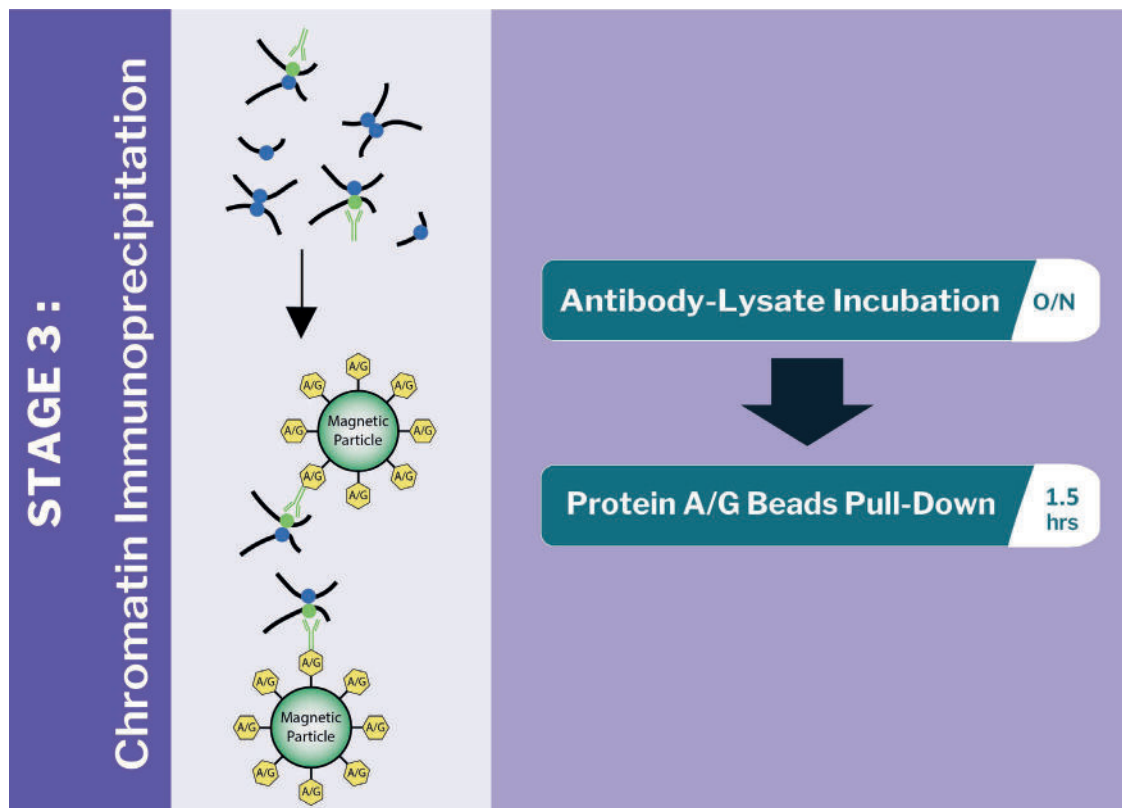

### Before You Begin

- » Dilute ● 10X RIPA to 1X with UltraPure Water. Store at room temperature. 1X RIPA is stable at room temperature for 2 months. You need ~4 mL of 1X RIPA per sample.

### 3.1 Antibody-Lysate Incubation

#### Follow the steps below for Antibody-Lysate Incubation:

1. Determine the amount of lysate to use for your antibody of interest (see table below for Dovetail validated antibodies).

**NOTE** For the antibody concentration information, please refer to the vendor's Certificate of Analysis for the antibody or contact the antibody vendor.

Antibody	Supplier	Part Number	Recommended amount (ng or $\mu$ L) of antibody	Recommended amount (ng) of chromatin (clarified lysate) input
IgG	Cell Signaling	2729	Equivalent amount as the antibody of interest	Equivalent amount as the antibody of interest
CTCF	Cell Signaling	3418	500 ng	1,000 - 1,500
H3K4ac	Active Motif	39381	7.5 $\mu$ L	1,000 - 1,500
H3K4me3	Cell Signaling	9751	1,250 ng	1,000 - 1,500
H3K14ac	Cell Signaling	7627	4,000 ng	1,000 - 1,500
H3K27ac	Cell Signaling	8173	300 ng	1,000 - 1,500
H3K27ac	Millipore Sigma	MABE647	200 ng	1,000 - 1,500
H3K27me3	Cell Signaling	9733	1,250 ng	1,000 - 1,500
H3K36me3	Cell Signaling	4909	1,250 ng	1,000 - 1,500
Poll	Abcam	ab26721	20,000 ng	1,000 - 1,500
Klf4	Abcam	ab106629	20,000 ng	10,000
Nanog	Abcam	ab21624	5,000 ng	10,000
Oct4	Cell Signaling	2890	25 $\mu$ L	10,000
Sox2	Cell Signaling	23064	500 ng	10,000

2. Place the appropriate amount of lysate into a new 1.5 mL tube.

#### NOTES

- » If the amount of lysate is < 200  $\mu$ L, bring the volume up to 200  $\mu$ L with **1X** RIPA + 25X Protease Inhibitors. This ensures you have sufficient volume for rotation with the antibody. For example, if the lysate amount is 100  $\mu$ L, bring it up to 200  $\mu$ L by adding 96  $\mu$ L of **1X** RIPA and 4  $\mu$ L of 25X Protease Inhibitors.
- » If multiple cell aliquots of the same sample were processed to reach the required clarified lysate amount, combine the lysates from these preparations at this step prior to incubating with the antibody.

3. Add the recommended amount of antibody (see table above) to the lysate in the 1.5 mL tube.
4. Invert to mix then rotate at 4°C overnight (at least 12 hours).

## 3.2 Protein A/G Beads Pull-down

Follow the steps below for Protein A/G Beads Pull-down:


1. Equilibrate the Protein A/G beads to room temperature.
2. Vortex the Protein A/G beads thoroughly (> 30 seconds) to resuspend the beads.
3. Transfer 25  $\mu$ L of resuspended Protein A/G beads to a new 1.5 mL tube.
4. Place the tube in the magnetic rack for 1 minute. Discard the supernatant.
5. Remove the tube from the magnetic rack and wash the beads with 200  $\mu$ L 1X RIPA. Pipet up and down to resuspend the beads and place the tube in the magnetic rack for 1 minute or until the solution looks clear. Discard the supernatant.
6. Repeat step 5 once, for a total of 2 washes.
7. After the last wash has been aspirated, remove the tube from the magnetic rack and resuspend the beads in 50  $\mu$ L 1X RIPA.
8. Quick spin your antibody-lysate complex that was incubated overnight (see step 4 in [3.1 Antibody-Lysate Incubation, page 21](#).) and add it to the tube containing the resuspended beads. Gently pipet up and down to fully mix, taking care to avoid creating bubbles.
9. Rotate at room temperature for 1 hour.
10. Quick spin the tube and place it in the magnetic rack for 1 minute or until the solution looks clear. Discard the supernatant.
11. Remove the tube from the magnetic rack and wash the beads with 1 mL 1X RIPA: pipet up and down to resuspend the beads, quick spin and place the tube in the magnetic rack for 2 minutes. Discard the supernatant.
12. Repeat step 11 twice, for a total of 3 washes.
13. Remove the tube from the magnetic rack and wash the beads with 1 mL 1X Wash Buffer: gently pipet up and down to resuspend the beads (taking care to avoid creating bubbles), quick spin and place the tube in the magnetic rack for 2 minutes. Discard the supernatant.
14. Repeat step 13 once, for a total of 2 washes.
15. Remove the tube from the magnetic rack and wash the beads with 1 mL 1X Wash Buffer: pipet up and down to resuspend the beads (gently, taking care to avoid creating bubbles), quick spin and place the tube in the magnetic rack. **Do not remove and discard the supernatant at this step yet.** Keep the tube in the magnetic rack and the beads in buffer to ensure they do not dry out while you prepare for the next reaction.
16. Continue to [Stage 4: Proximity Ligation, page 23](#).

## Stage 4: Proximity Ligation

As you prepare for Stage 4, keep the following in mind:

- » Proximity ligation takes ~ 4 hours.
- » Follow best practices when working with beads (see [Good Practices, page 8](#)).

Figure 5. Stage 4: Proximity Ligation

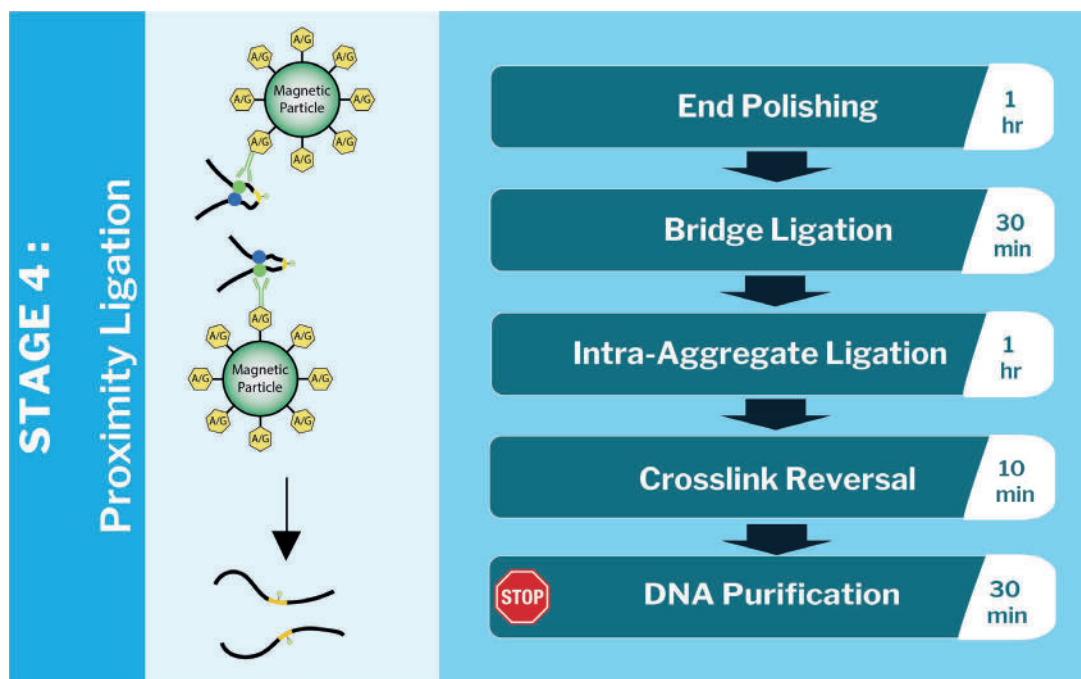

### Before You Begin

- » The ● Crosslink Reversal Buffer might have precipitated in storage. Incubate at 37°C for 15 minutes or until the precipitate is no longer visible. Vortex to mix prior to use.
- » Thaw ● End Polishing Buffer, ● 5X Bridge Ligation Buffer, ● Bridge, and ● Intra-Aggregate Ligation Buffer at room temperature. Leave on ice once thawed. Vortex to mix prior to use.

## 4.1 End Polishing

Follow the steps below for End Polishing:

1. Aspirate and discard the supernatant from step 15 in [3.2 Protein A/G Beads Pull-down, page 22](#). Remove the tube from the magnetic rack and add to the beads 53  $\mu\text{L}$  of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
● End Polishing Buffer	50 $\mu\text{L}$	55 $\mu\text{L}$	x	8	=	440 $\mu\text{L}$
● End Polishing Enzyme Mix	3 $\mu\text{L}$	3.3 $\mu\text{L}$	x	8	=	26.4 $\mu\text{L}$
<b>Total</b>	<b>53 <math>\mu\text{L}</math></b>					

2. Pipet up and down to fully mix then transfer the sample to a **new 1.5 mL tube**.
3. Incubate in an agitating thermal mixer set at 1,250 rpm as follows:

Temperature	Time
22°C	30 minutes
65°C	30 minutes

4. Allow the tube to reach room temperature then quick spin, and place it in the magnetic rack for 1 minute (or until the solution looks clear). Discard the supernatant.
5. Remove the tube from the magnetic rack and wash the beads once with 150  $\mu\text{L}$  1X Wash Buffer. Pipet up and down to resuspend the beads, place the tube in the magnetic rack. **Do not remove and discard the supernatant at this step yet.** Keep the tube in the magnetic rack and the beads in buffer to ensure they do not dry out while you prepare for the next reaction.

## 4.2 Bridge Ligation

Follow the steps below for Bridge Ligation:

1. Prepare and place on ice **fresh** 50  $\mu\text{L}$  Bridge Ligation Mix by mixing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	35 $\mu\text{L}$	38.5 $\mu\text{L}$	x	8	=	308 $\mu\text{L}$
● 5X Bridge Ligation Buffer	10 $\mu\text{L}$	11 $\mu\text{L}$	x	8	=	88 $\mu\text{L}$
● Bridge	5 $\mu\text{L}$	5.5 $\mu\text{L}$	x	8	=	44 $\mu\text{L}$
<b>Total</b>	<b>50 <math>\mu\text{L}</math></b>					

2. Aspirate and discard the supernatant from step 5 in [4.1 End Polishing, page 24](#). Remove the tube from the magnetic rack and add to the beads:



Reagent	Volume Per Reaction
Bridge Ligation Mix	50 $\mu$ L
● Bridge Ligase	1 $\mu$ L
<b>Total</b>	<b>51 <math>\mu</math>L</b>

- Pipet up and down to fully mix. Incubate at 22°C for 30 minutes in an agitating thermal mixer set at 1,250 rpm.
- Quick spin the tube, then place it in the magnetic rack for 1 minute (or until the solution looks clear). Discard the supernatant.
- Remove the tube from the magnetic rack and wash the beads once with 150  $\mu$ L 1X Wash Buffer. Pipet up and down to resuspend the beads, place the tube in the magnetic rack for 1 minute and discard the supernatant.

## 4.3 Intra-Aggregate Ligation

Follow the steps below for Intra-Aggregate Ligation:

- Remove the tube from the magnetic rack and add to the beads 52  $\mu$ L of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
● Intra-Aggregate Ligation Buffer	50 $\mu$ L	55 $\mu$ L	x	8	=	440 $\mu$ L
● Intra-Aggregate Ligation Enzyme Mix	2 $\mu$ L	2.2 $\mu$ L	x	8	=	17.6 $\mu$ L
<b>Total</b>	<b>52 <math>\mu</math>L</b>					

- Pipet up and down to fully mix. Incubate at 22°C for 1 hour in an agitating thermal mixer set at 1,250 rpm.



**SAFE STOP** For convenience, this ligation reaction can proceed overnight at 22°C in an agitating thermal mixer set at 1,250 rpm.

- Quick spin the tube, then place it in the magnetic rack for 1 minute (or until the solution looks clear). Discard the supernatant.

## 4.4 Crosslink Reversal

Follow the steps below for Crosslink Reversal:

- Remove the tube from the magnetic rack and add to the beads 51.5  $\mu$ L of a master mix containing the following reagents **in the order listed**:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
● Crosslink Reversal Buffer	50 µL	55 µL	x	8	=	440 µL
● Proteinase K	1.5 µL	1.65 µL	x	8	=	13.2 µL
<b>Total</b>	<b>51.5 µL</b>					

2. Pipet up and down to fully mix. Incubate in an agitating thermal mixer set at 1,250 rpm as follows:

Temperature	Time
78°C	10 minutes
25°C	Hold



**SAFE STOP** For convenience, you can hold at 25°C overnight in an agitating thermal mixer set at 1,250 rpm.


3. Place the tube in the magnetic rack for 1 minute. Transfer 50 µL of the **SUPERNATANT** to a new 1.5 mL tube. Discard the beads.


## 4.5 DNA Purification

### Follow the steps below for DNA Purification:

1. Vortex the SPRIselect beads thoroughly (>30 seconds) to resuspend.
2. Add 90 µL of resuspended SPRIselect beads to the 1.5 mL tube containing your sample.
3. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
4. Incubate the tube at room temperature, off the magnetic rack, for 10 minutes.
5. Quick spin the tube and place it in the magnetic rack for 5 minutes. Discard the supernatant.
6. Leave the tube in the magnetic rack and wash the beads **twice** with 200 µL **fresh** 80% ethanol. Do not resuspend the beads for these washes. Add the ethanol, wait for 1 minute then discard the ethanol supernatant.
7. After the last wash, quick spin the tube and place it in the magnetic rack for 1 minute. Use a 10 µL pipet tip to remove traces of ethanol
8. Air dry the beads in the magnetic rack for 5 minutes until no residual ethanol remains. **Do not over dry the beads.**
9. Off the magnetic rack, resuspend the beads in 57 µL TE Buffer pH 8.0.
10. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
11. Incubate at room temperature, off the magnetic rack, for 5 minutes.
12. Quick spin the tube and place it in the magnetic rack for 1 minute (or until the solution looks clear).
13. Transfer 55 µL of the **SUPERNATANT** (purified DNA) to a new tube. Discard the beads.

14. Quantify 5  $\mu$ L of your purified DNA using a Qubit Fluorometer and Qubit dsDNA HS Kit. The amount of DNA recovered is dependent on the antibody used, and in some cases, may be below the detection limit.

 **NOTE** The amount of DNA recovered after purification determines the adaptor dilution during library preparation (Stage 5) and number of PCR cycles (Stage 6). This purified DNA will go into library preparation and will also be referred to as DNA input.


 **SAFE STOP** Purified DNA sample can be stored at  $-20^{\circ}\text{C}$  for up to 6 months.

## Stage 5: Library Preparation

As you prepare for Stage 5, keep the following in mind:

- » The library preparation protocol does not require fragmentation.
- » The library preparation protocol takes ~ 2 hours.
- » Follow best practices when working with beads (see [Good Practices, page 8](#)).

Figure 6. Stage 5: Library Preparation

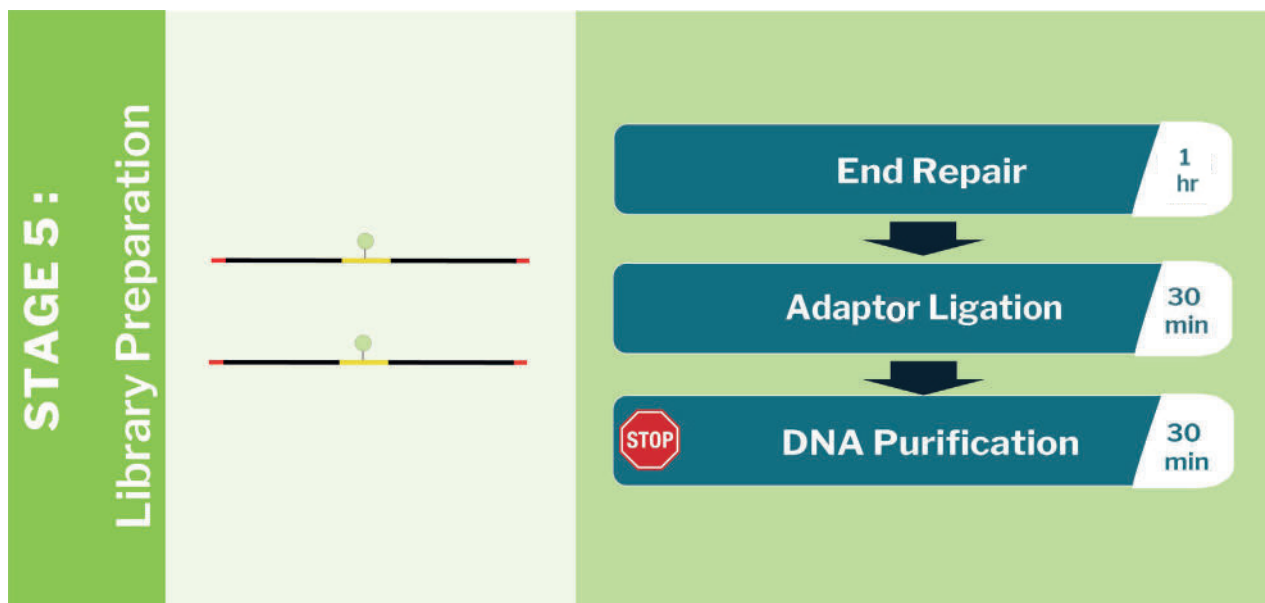

### Before You Begin

- » The ● End Repair Buffer may have precipitated in storage. Incubate for at least 10 minutes at 37°C until there is no visible precipitate.
- » Thaw ● 250 mM DTT and ● Adaptor for Illumina at room temperature. Vortex to mix prior to use.

## 5.1 End Repair

Follow the steps below for End Repair:

1. Place the 50  $\mu\text{L}$  of purified DNA input in a 0.2 mL PCR tube.
2. Add to the PCR tube 10.5  $\mu\text{L}$  of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
● End Repair Buffer	7 $\mu\text{L}$	7.7 $\mu\text{L}$	x	8	=	61.6 $\mu\text{L}$
● End Repair Enzyme Mix	3 $\mu\text{L}$	3.3 $\mu\text{L}$	x	8	=	26.4 $\mu\text{L}$
● 250 mM DTT	0.5 $\mu\text{L}$	0.6 $\mu\text{L}$	x	8	=	4.8 $\mu\text{L}$
<b>Total</b>	<b>10.5 <math>\mu\text{L}</math></b>					

3. Pipet up and down to fully mix. Quick spin the tube.
4. Place in a thermal cycler, with the heated lid set to  $\geq 75^{\circ}\text{C}$ , and run the following program:

Temperature	Time
20°C	30 minutes
65°C	30 minutes
12°C	Hold

## 5.2 Adaptor Ligation and USER Digest

Follow the steps below for Adaptor Ligation and USER Digest:

1. Determine whether adaptor dilution is necessary. If DNA input is < 5 ng, dilute the ● Adaptor for Illumina in 10 mM Tris-HCl, pH 7.5 containing 10 mM NaCl, as indicated below.

Input	Adaptor Dilution
500 ng – 5 ng	No Dilution
< 5 ng	2.5-fold (1:2.5)

2. Add to the PCR tube containing the end-repaired sample the following reagents:

Reagent	Volume Per Reaction
● Adaptor for Illumina (or diluted Adaptor if DNA input < 5 ng)	2.5 µL
● Ligation Enzyme Mix	30 µL
● Ligation Enhancer	1 µL
<b>Total</b>	<b>33.5 µL</b>

**NOTE** The Ligation Enzyme Mix and Ligation Enhancer can be mixed ahead of time. The master mix is stable for 8 hours at 4°C. We do not recommend adding the Adaptor for Illumina to the master mix.

3. Pipet up and down to fully mix. Quick spin the tube.
4. Incubate at 20°C for 15 minutes in a thermal cycler with the heated lid off. Hold at 12°C.
5. Following incubation, add 3 µL of ● USER Enzyme Mix to the PCR tube.
6. Pipet up and down to fully mix. Quick spin the tube.
7. Incubate at 37°C for 15 minutes in a thermal cycler with the heated lid set to ≥ 47°C. Hold at 12°C.

## 5.3 DNA Purification

### Follow the steps below for DNA Purification:

1. Vortex the SPRIselect beads thoroughly (>30 seconds) to resuspend.
2. Add 80  $\mu$ L of resuspended SPRIselect beads to the PCR tube containing the adaptor-ligated sample.
3. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
4. Incubate the tube at room temperature, off the magnetic rack, for 10 minutes.
5. Quick spin the tube and place it in the magnetic rack for 5 minutes. Discard the supernatant.
6. Leave the tube in the magnetic rack and wash the beads **twice** with 200  $\mu$ L **fresh** 80% ethanol. Do not resuspend the beads for these washes. Add the ethanol, wait for 1 minute then discard the ethanol supernatant.
7. Quick spin the tube and place it in the magnetic rack for 1 minute. Use a 10  $\mu$ L pipet tip to remove traces of ethanol.
8. Air dry the beads in the magnetic rack for 5 minutes until no residual ethanol remains. **Do not over dry the beads.**
9. Off the magnetic rack, resuspend the beads in 22  $\mu$ L TE Buffer pH 8.0.
10. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
11. Incubate at room temperature, off the magnetic rack, for 5 minutes.
12. Quick spin the tube and place it in the magnetic rack for 1 minute (or until the solution looks clear).
13. Transfer 20  $\mu$ L of the **SUPERNATANT** (purified adaptor-ligated DNA) to a new tube. Discard the beads.




**SAFE STOP** Purified DNA sample can be stored at -20°C overnight.

## Stage 6: Ligation Capture and Amplification

As you prepare for Stage 6, keep the following in mind:

- » The Ligation Capture and Amplification protocol takes ~ 2 hours.
- » Follow best practices when working with beads (see [Good Practices, page 8](#)).

Figure 7. Stage 6: Ligation Capture and Amplification

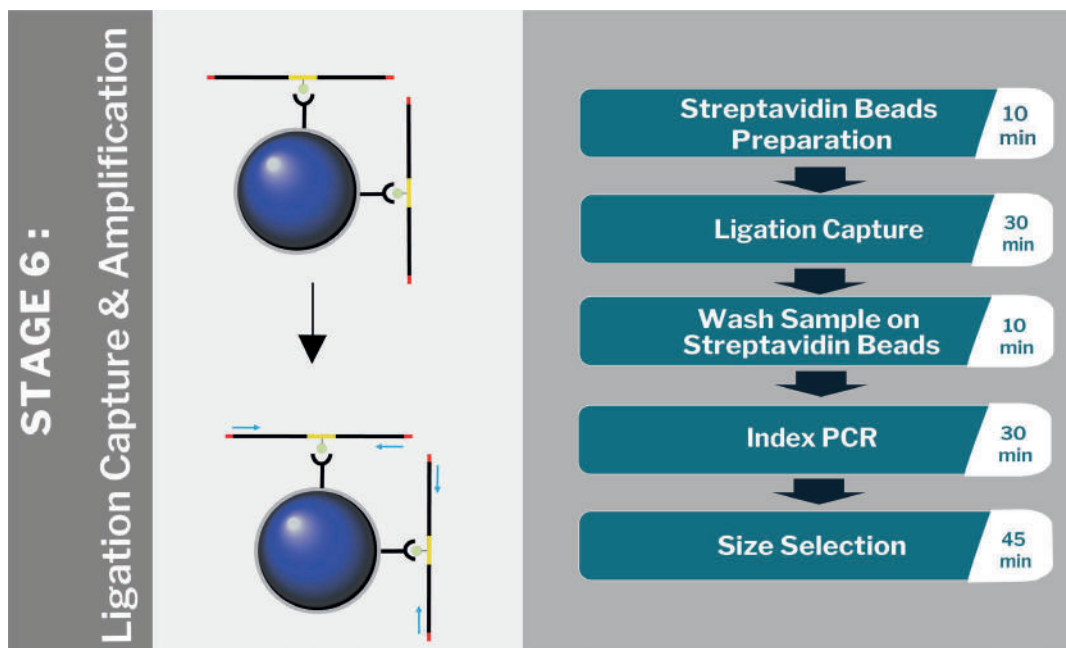

### Before You Begin




- » Thaw ● UDI Primer Pair and HotStart PCR Ready Mix and **keep on ice while in use**. Vortex to mix prior to use.
- » Equilibrate ● Streptavidin Beads and ■ NWB at room temperature

### 6.1 Streptavidin Beads Preparation

**NOTE** This step does not involve any DNA sample.



## Follow the steps below for Ligation Capture and Amplification:


1. Vortex the  Streptavidin Beads vial thoroughly (> 30 seconds) to resuspend the beads. Transfer 25  $\mu$ L of resuspended  Streptavidin beads to a new 1.5 mL tube.
2. Place the 1.5 mL tube containing the beads in the magnetic rack for 1 minute (or until the solution looks clear). Discard the supernatant.
3. Remove the tube from the magnetic rack and wash the beads with 200  $\mu$ L of 1X Wash Buffer: pipet up and down to resuspend the beads and place the tube in the magnetic rack for 1 minute (or until the solution looks clear). Discard the supernatant.
4. Repeat step 3 once, for a total of 2 washes.
5. After the second wash, resuspend the beads in 100  $\mu$ L  NWB. Pipet up and down to fully mix.
6. Transfer to a 0.2 mL PCR tube.

## 6.2 Ligation Capture


### Follow the steps below for Ligation Capture:

1. Transfer the 20  $\mu$ L of purified adaptor-ligated DNA (from step 13 in [5.3 DNA Purification, page 31](#)) to the 0.2 mL tube containing the Streptavidin beads resuspended in 100  $\mu$ L of NWB.
2. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
3. Incubate at 25°C for 30 minutes in an agitating thermal mixer set at 1,250 rpm (or on the bench with no shaking, if an agitating thermal mixer for 0.2 mL tubes is not available).

## 6.3 Wash Sample on Streptavidin Beads

 **NOTE** For each of the washes below, remove the tube from the magnetic rack, add the indicated buffer to the beads, pipet up and down to resuspend the beads, place the tube in the magnetic rack for 1 minute (or until the solution looks clear), and discard the supernatant. Remove all of the supernatant between each wash; residual supernatant can interfere with the downstream PCR.

### Follow the steps below for Wash Sample on Streptavidin Beads:

1. Quick spin the tube and place it in the magnetic rack for 1 minute. Discard the supernatant.
2. Wash the beads **twice** with 200  $\mu$ L  NWB.
3. Wash the beads **twice** with 200  $\mu$ L 1X Wash Buffer.

## 6.4 Index PCR

**NOTE** Not all PCR enzymes and master mixes are compatible for amplification in the presence of Streptavidin beads. Please use the HotStart PCR Ready Mix supplied in your Dovetail Kit. (Box 2).

### Follow the steps below for Index PCR:

1. After the last wash, remove the tube from the magnetic rack and add to the beads 45  $\mu$ L of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	20 $\mu$ L	22 $\mu$ L	x	8	=	176 $\mu$ L
HotStart PCR Ready Mix	25 $\mu$ L	27.5 $\mu$ L	x	8	=	220 $\mu$ L
<b>Total</b>	<b>45 <math>\mu</math>L</b>					

2. Add 5  $\mu$ L ● UDI Primer Pair to the PCR reaction. Use one UDI Primer Pair per PCR reaction (see [Appendix 2: Dual Index Primers, page 40](#)).
3. Pipet up and down to fully mix.
4. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle). Place the tube into the thermal cycler and run the following program:

Step	Temperature	Time	Cycles
Enzyme Activation	98°C	3 minutes	1
Denature	98°C	20 seconds	See table below
Anneal	65°C	20 seconds	
Extend	72°C	30 seconds	
Extend	72°C	1 minute	1
	12°C	Hold	1

DNA Input (Stage 4.5, Step 14)	Cycles
$\geq 100$ ng	12
< 100 ng - 5 ng	14
< 5 ng	16
undetected	18

## 6. 5 Size Selection


Follow the steps below for Size Selection:

1. Quick spin the PCR tube and place it in the magnetic rack for 1 minute.
2. Transfer 50  $\mu$ L of the **SUPERNATANT** to a new 1.5 mL tube. Discard the beads.
3. Add 50  $\mu$ L of TE Buffer pH 8.0 to the 1.5 mL tube to bring the volume of the sample in the tube to 100  $\mu$ L.
4. Vortex the SPRIselect beads thoroughly (>30 seconds) to resuspend.
5. Add 50  $\mu$ L of resuspended SPRIselect beads to the 1.5 mL tube containing your sample.
6. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
7. Incubate the tube at room temperature, off the magnetic rack, for 10 minutes.
8. Quick spin the tube and place it in the magnetic rack for 5 minutes.
9. Transfer 145  $\mu$ L of the **SUPERNATANT** to a new 1.5 mL tube. Discard the beads.
10. Add 30  $\mu$ L of resuspended SPRIselect beads to the 1.5 mL tube containing your sample.
11. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
12. Incubate the tube at room temperature, off the magnetic rack, for 10 minutes.
13. Quick spin the tube and place it in the magnetic rack for 5 minutes. Discard the supernatant.
14. Leave the tube in the magnetic rack and wash the beads **twice** with 200  $\mu$ L **fresh** 80% ethanol. Do not resuspend the beads for these washes. Add the ethanol, wait for 1 minute then discard the ethanol supernatant.
15. Quick spin the tube and place it in the magnetic rack for 1 minute. Use a 10  $\mu$ L pipet tip to remove traces of ethanol.
16. Air dry the beads in the magnetic rack for 5 minutes until no residual ethanol remains. **Do not over dry the beads.**
17. Off the magnetic rack, resuspend the beads in 30  $\mu$ L TE Buffer pH 8.0.
18. Vortex to mix thoroughly. Quick spin the tube (make sure to spin down only briefly and to stop before the beads start to settle).
19. Incubate the tube at room temperature, off the magnetic rack, for 5 minutes.
20. Quick spin the tube and place it in the magnetic rack for 1 minute (or until the solution looks clear).
21. Transfer 28  $\mu$ L of the **SUPERNATANT** to a new 1.5 mL tube. The supernatant is your size selected library. Discard the beads.
22. Quantify your size selected library using a Qubit Fluorometer and Qubit dsDNA HS Kit.
23. Use a TapeStation or Bioanalyzer to verify the size distribution of your size selected library. The size range is expected to be between 350 bp and 1,000 bp (Figure 8).



**SAFE STOP** The library can be stored at -20°C for up to 6 months.

Figure 8. Expected final library profile, as analyzed on HS D5000 ScreenTape.

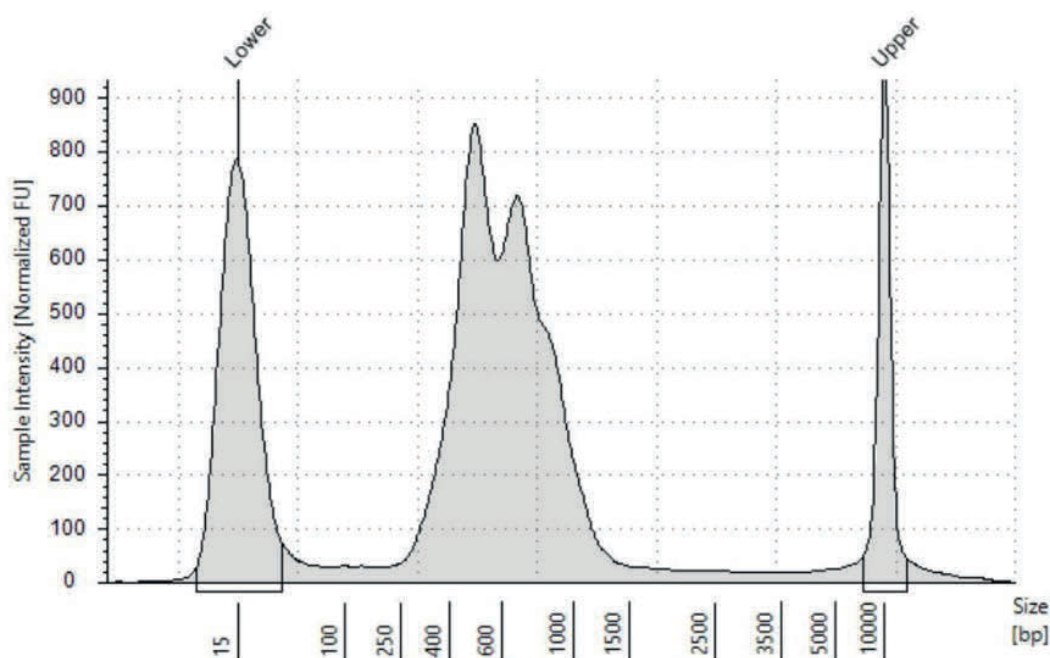

## Sequencing & QC Analysis

Dovetail® HiChIP MNase libraries are sequenced via Illumina® sequencers in paired-end mode. Each library can be sequenced to ~150 M read pairs. We recommend to shallow sequence the library to run a QC analysis prior to deep sequencing. The QC analysis requires ~20 M read pairs (2 x 150 bp). Cantata Bio provides all kit users access to a QC analysis workflow available on readthedocs: <https://hichip.readthedocs.io/en/latest/>.

## Appendix 1: Sample Preparation for $1 \times 10^6$ Cell Input

As you prepare for  $1 \times 10^6$  cell input, keep the following in mind:

- » Sample preparation takes 1.5 hours.

### Before You Begin

- » The 10X Wash Buffer and 20% SDS might have precipitated in storage. Incubate these solutions at 37°C for 15 minutes or until the precipitate is no longer visible. Vortex to mix prior to use.
- » Dilute 10X Wash Buffer to 1X with UltraPure™ Water. Store at room temperature. 1X Wash Buffer is stable at room temperature for 2 months. You need ~6 mL of 1X Wash Buffer per sample for the entire protocol.
- » Prepare 0.3 M DSG in DMSO (anhydrous) by dissolving 1 mg of DSG in 10.22  $\mu$ L DMSO. DSG is water-insoluble and moisture-sensitive. Prepare **immediately** before use. Do not store DSG in solution.
- » Prepare 25X Proteinase Inhibitors by dissolving 1 tablet of cOmplete™ Protease Inhibitor Cocktail in 2 mL of UltraPure™ Water and place on ice. The 25X Proteinase Inhibitors solution is stable at 4°C for 2 weeks.
- » Prepare fresh 1X Nuclease Digest Buffer and store at room temperature. 1X Nuclease Digest Buffer is stable for 1 day at room temperature. You need 50  $\mu$ L of 1X Nuclease Digest Buffer per sample. To prepare 1X Nuclease Digest Buffer (50  $\mu$ L), mix the following components:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	40 $\mu$ L	44 $\mu$ L	x	8	=	352 $\mu$ L
10X Nuclease Digest Buffer	5 $\mu$ L	5.5 $\mu$ L	x	8	=	44 $\mu$ L
100 mM MgCl <sub>2</sub>	5 $\mu$ L	5.5 $\mu$ L	x	8	=	44 $\mu$ L
<b>Total</b>	<b>50 <math>\mu</math>L</b>					

- » Set the thermal mixer at 22°C, shaking at 1,250 rpm.
- » Thaw 0.5 M EGTA at room temperature. Vortex to mix prior to use.

## Crosslinking and Digestion

### NOTES

- »  $1 \times 10^6$  cells are needed per HiChIP reaction.
- » Pre-freezing the cells is required to get an optimal digestion profile.
- » The cell pellet should be frozen at  $-80^\circ\text{C}$  for at least 30 minutes (step 4). You can keep the cells frozen at  $-80^\circ\text{C}$  for longer provided they are not subjected to freeze-thaw.
- » All crosslinking reactions (steps 5 – 12) should be carried out at room temperature.

### Follow the steps below for Crosslinking and Digestion:

1. Harvest the cells, wash with 1X PBS and count.
2. Aliquot  $1 \times 10^6$  cells into a 1.5 mL tube.
3. Spin the  $1 \times 10^6$  cell aliquot at  $500 \times g$  for 5 minutes in a swinging bucket rotor. Carefully discard the supernatant.
4. Freeze the cell pellet by placing it at  $-80^\circ\text{C}$  for at least 30 minutes.
5. Thaw your cell pellet quickly at room temperature then resuspend the pellet in 200  $\mu\text{L}$  of 1X PBS: first add 50  $\mu\text{L}$  of 1X PBS and pipet up and down to break up clumps then add the remaining 150  $\mu\text{L}$ . Pipet up and down to fully resuspend the pellet.
6. Add 2  $\mu\text{L}$  of 0.3 M DSG. **Pipet up and down to mix.**
7. Rotate the tube for 10 minutes at room temperature. Cells should not settle.
8. Add 5.4  $\mu\text{L}$  of 37% formaldehyde.
9. Rotate the tube for 10 minutes at room temperature. Cells should not settle.
10. Spin the tube at  $500 \times g$  for 5 minutes in a swinging bucket rotor. Carefully discard the supernatant. Use caution, the pellet might be loose.
11. Wash the pellet with 200  $\mu\text{L}$  of 1X Wash Buffer, pipet up and down to break up clumps and fully resuspend the pellet.
12. Spin the tube at  $500 \times g$  for 5 minutes in a swinging bucket rotor. Carefully discard the supernatant.
13. Repeat steps 11 and 12 once, for a total of 2 washes.
14. After removing the second wash, resuspend the cell pellet in 50  $\mu\text{L}$  1X Nuclease Digest Buffer (freshly prepared, see [Before You Begin, page 37](#)).
15. Add 0.5  $\mu\text{L}$  of MNase Enzyme Mix and pipet up and down to fully mix.
16. Incubate the tube at  $22^\circ\text{C}$  for exactly 15 minutes in an agitating thermal mixer set at 1,250 rpm. If you are working with a large number of samples, stagger the start of the digestion for each sample by 20 seconds then stop after corresponding 15 minutes.
17. Stop the reaction by adding 5  $\mu\text{L}$  of ● 0.5 M EGTA. Pipet up and down to fully mix.

## RIPA Cell Lysis

### Follow the steps below for RIPA Cell Lysis:

1. Add to the sample tube 144.5 µL of a master mix containing the following reagents:

Reagent	Volume Per Reaction	10% Extra		# Reactions		Final
UltraPure Water	115.5 µL	127.1 µL	x	8	=	1,016.8 µL
● 10X RIPA	20 µL	22 µL	x	8	=	176 µL
25X Protease Inhibitors	8 µL	8.8 µL	x	8	=	70.4 µL
● 20% SDS	1 µL	1.1 µL	x	8	=	8.8 µL
<b>Total</b>	<b>144.5 µL</b>					

2. Vortex the tube to mix three times for 5 seconds each.
3. Rotate the tube at room temperature for 15 minutes.
4. Spin the tube at 16,000 x g for 2 minutes.
5. Transfer the **SUPERNATANT (clarified lysate)** to a new 1.5 mL tube. This lysate contains the digested chromatin.
6. Continue to [Stage 2: Lysate QC, page 16](#).

## Appendix 2: Dual Index Primers

Dovetail® Dual Index Primer Set #1 for Illumina® includes the following eight UDI Primer Pairs:

**Table 7. UDI Primer Pairs**

Primer Name	HiSeq® 2000/2500, MiSeq®, NovaSeq® systems	HiSeq® 3000, 4000, X, NextSeq®, MiniSeq®, iSeq® systems	All Systems
	i5 index	i5 index	i7 index
UDI Primer Pair 1	ATATGCGC	GCGCATAT	CTGATCGT
UDI Primer Pair 2	TGGTACAG	CTGTACCA	ACTCTCGA
UDI Primer Pair 3	AACCGTTC	GAACGGTT	TGAGCTAG
UDI Primer Pair 4	TAACCGGT	ACCGGTTA	GAGACGAT
UDI Primer Pair 5	GAACATCG	CGATGTTC	CTTGTCGA
UDI Primer Pair 6	CCTTG TAG	CTACAAGG	TTCCAAGG
UDI Primer Pair 7	TCAGGCTT	AAGCCTGA	CGCATGAT
UDI Primer Pair 8	GTTCTCGT	ACGAGAAC	ACGGAACA

The indexes on the UDI Primer Pairs are color-balanced in sets of four (1-4, 5-8). Indexes within each group of four are fully color balanced and can be pooled for sequencing. You can multiplex less than four samples, but verify color balance before pooling.